

Dräger DrugTest 5000 Test Kit


Screening for drugs of abuse in oral fluid

The Dräger DrugTest 5000 system consists of two main components: The DrugTest 5000 test kits and the DrugTest 5000 Analyzer. It is a fast and highly accurate system for testing saliva (oral fluid) samples for substances such as amphetamines, designer amphetamines, opiates, cocaine and its metabolites, benzodiazepines, cannabinoids, ketamine or methadone.

Dräger

Technology for Life

Dräger DrugTest 5000 Test Kit

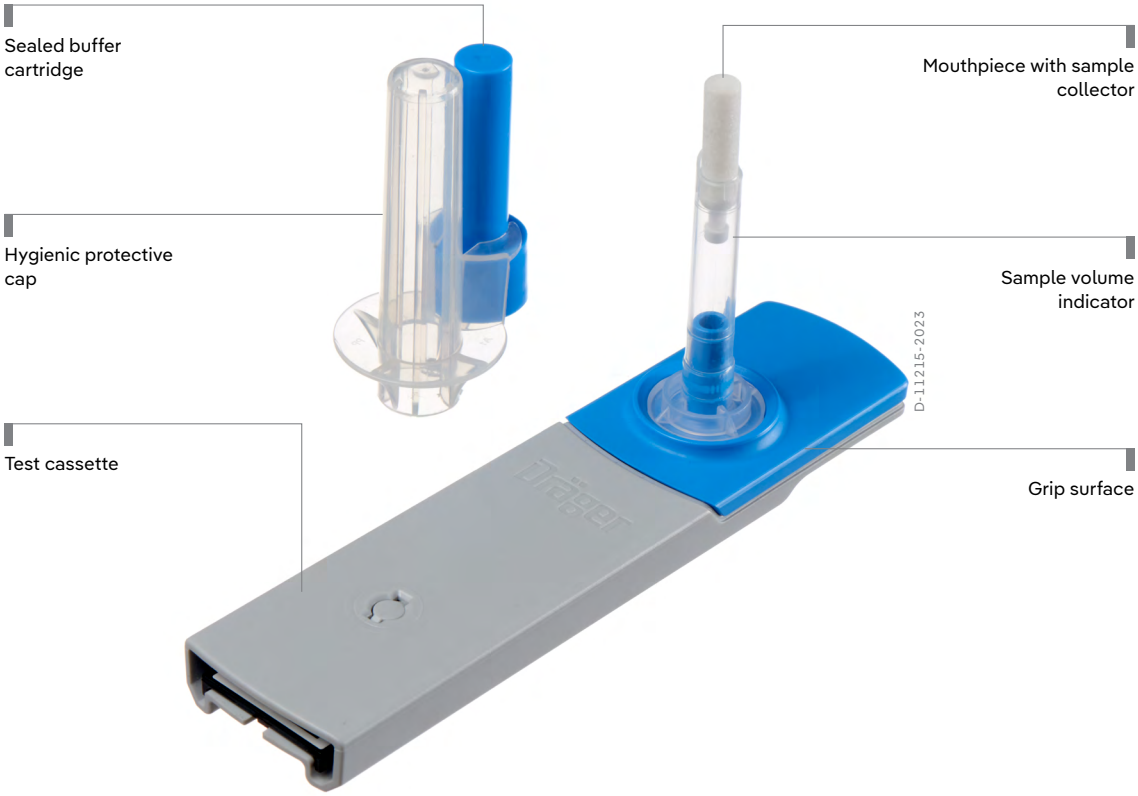

Benefits

Ergonomic and Easy to Use

The DrugTest 5000 test kits are ergonomically designed, easy to handle, and immediately ready for use. The kit consists of a test cassette and a sample collector. Can be handled with or without gloves by both right-handed and left-handed persons.

Clear and Reliable Results

The test result is clearly displayed, making misinterpretation impossible. The test cassette can be labelled with the subject's name and the date, making it easier to match samples to subjects.

Hygienic and Non-Invasive Sampling

Made from rigid porous material with capillary properties. Non-invasive test allows for hygienic handling. Any contact with the sample and its components is prevented.


Simple and Error-Proof Procedure

The test is performed in a few simple steps, excluding incorrect operation. The straightforward procedure and integrated indicator ensure proper sample collection: The indicator turns blue when enough liquid is absorbed.

Rapid Testing and Versatile Application


The entire sampling process is supervised by the operator, and once the analysis is finalised, the result is clearly displayed. It can be used in conjunction with the Dräger DCD 5000 saliva (oral fluid) sample collector to take a second sample and to store or transport samples for laboratory analysis. In combination with the Dräger SSK 5000, it takes only a few minutes to determine whether a suspicious surface, preparation, or substance may be associated with designated types of narcotics.

Details

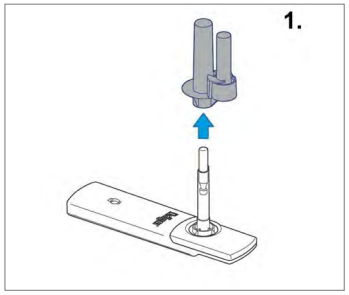


D-2315-2026

Remove the safety cap with the cartridge and keep it for later use

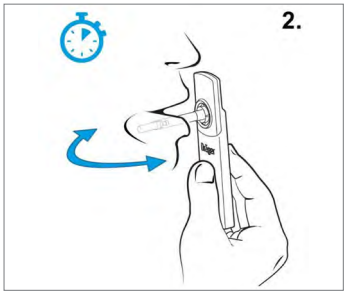


D-2316-2026

Insert the sample collector into the mouth to actively collect oral fluid

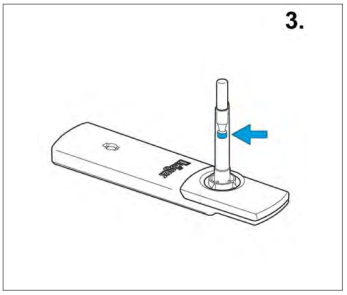


D-2317-2026

The integrated indicator turns blue once a sufficient sample has been collected

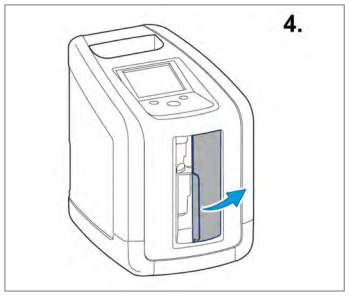


D-2318-2026

Open the analyzer door

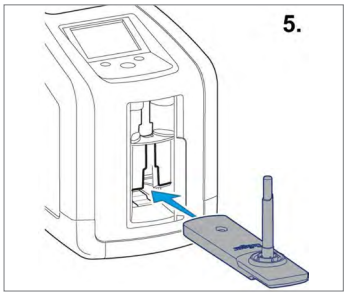


D-2319-2026

Insert the test cassette into the lower insertion slot of the analyzer

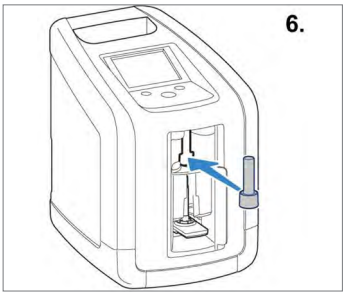


D-2320-2026

Remove the cartridge from the safety cap and insert it into the upper slot of the analyzer

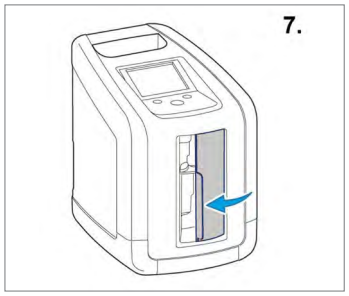

D-2321-2026

Close the door

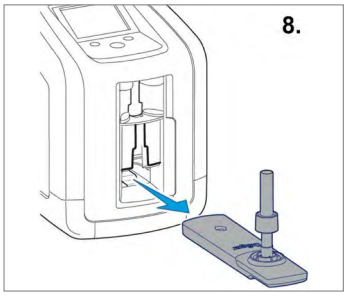

D-2322-2026

After the analysis is complete, remove the test cassette with the attached cartridge from the analyzer

Accessories



D-6296-2009

SSK 5000

Ideal for surface drug testing applications, the SSK 5000 sampling system is quick and easy to use. When used with the DrugTest 5000, the sample can be transferred to a test cassette and screened for possible drug contamination. The sample can also be stored and transported for further testing.



ST-13225-2007

DCD 5000

Simple, fast and secure detection of intoxicants and drugs: The DCD 5000 does not only enable an easy collection of saliva (oral fluid), the samples can be stored and sent to the laboratory for analysis – without the sample being falsified along the way.



D-15278-2017

SCK

The SCK confirmation set contains two samplers and stabilising components (isopropanol) as well as documentation forms and shipping materials, ensuring a chain of custody through clear documentation and secure shipment of samples to the lab.

Related Products



D-54720-2012

DrugTest 5000

No pipetting, no drips, no timing: With the DrugTest 5000, a drug test is carried out simply and quickly. The collected saliva (oral fluid) sample can be analysed immediately – for an accurate result on the spot.



D-16484-2024

Dräger DrugCheck 3000

Use the DrugCheck 3000 to find out within minutes whether a person has recently consumed certain drugs. The compact and quick saliva (oral fluid)-based drug test delivers reliable results affordably and easily. The non-invasive drug test kit does not require electricity and can therefore be used anywhere.

Technical Data

Test for detecting drugs in oral fluid	
Storage / transportation	4 °C to 30 °C (39 °F to 86 °F)

Ordering Information

Description	Part/Order Number
Each Dräger DrugTest 5000 test kit consists of a sample collector test cassette and a cartridge, packaged in a foil pouch.	
Test Kits for 8 Substances IVD: COC, OPI, BZO, THC, AMP, MET, MTD, KET* Standard: COC, OPI, BZO, THC, AMP, MET, MTD, KET*	 8323646** 3706092
Test Kits for 7 Substances IVD: COC, OPI, BZO, THC, AMP, MET, MTD* Standard: COC, OPI, BZO, THC, AMP, MET, MTD*	 8323156 8323636
Test Kits for 6 Substances IVD: COC, OPI, BZO, THC, AMP, MET* Standard: COC, OPI, BZO, THC, AMP, MET*	 8319830 8319965
Test Kits for 5 Substances IVD: COC, OPI, BZO, THC, AMP, MET* Standard: COC, OPI, BZO, THC, AMP, MET*	 8319830 8319965
Test Kits for Training (6 test kits each) Training test kits (3 x Positive, 3 x Negative)	 8323640
*COC: cocaine – *OPI: opiates – *BZO: benzodiazepines – *THC: tetrahydrocannabinol (cannabis) – *AMP: amphetamine – *MET: methamphetamine + designer amphetamines – *MTD: methadone – *KET: ketamine **Only sold within the European Union	
IVD version: Sales only as in-vitro-diagnostic device. Device placed on the market under the transitional provisions of Regulation (EU) 2017/746 (IVDR), in accordance with Article 110. Previously certified under Directive 98/79/EC. Standard version: Sales for forensic applications, use by lay persons and for workplace use.	
Accessories	
Dräger SSK 5000 Surface Test Kit	8320490
Dräger DCD 5000 Saliva Sample Collector	8319910
Dräger SCK Saliva Confirmation Kit for laboratory analysis	8323880
Dräger SCSK Saliva Confirmation Single Kit for laboratory analysis	8326300
Diagnostics carrying bag	8322675
Transport case	8325333
Keyboard “compact” QWERTZ (German)	8315095
Keyboard “compact” QWERTY (English)	8315497
Keyboard “compact” AZERTY (French)	8315142

Not all products, features, or services are for sale in all countries. Trademarks mentioned herein are the property of its respective owner. Trademarks may be owned by Drägerwerk AG & Co. KGaA (Dräger) or its affiliates in certain countries and not necessarily in the country in which this material is released. Visit www.draeger.com/trademarks for the current status of Dräger's trademarks.

Corporate Headquarters
Drägerwerk AG & Co. KGaA
Moislinger Allee 53–55
23558 Lübeck, Germany
www.draeger.com

Region Europe
Dräger Safety AG & Co. KGaA
Revalstraße 1
23560 Lübeck, Germany
+49 451 882 0
+49 451 882 2080
info@draeger.com

Region Asia Pacific
Draeger Singapore Pte. Ltd.
61 Science Park Road
The Galen #04-01
Singapore 117525
+65 6872 9288
+65 6259 0398

Region Middle East, Africa
Dräger Safety AG & Co. KGaA
Branch Office
P.O. Box 505108
Dubai, United Arab Emirates
+971 4 4294 600
+971 4 4294 699
contactuae@draeger.com

Region Central and South America
Dräger Safety do Brasil Ltda.
Al. Pucuruí, 51/61 – Tamboré
06460-100 Barueri, São Paulo
+55 (11) 4689-4900
relacionamento@draeger.com

Locate your Regional Sales Representative at:
www.draeger.com/contact

101310 | 00.14 | Subject to modifications | © 2026/04/23 Drägerwerk AG & Co. KGaA